


1/14

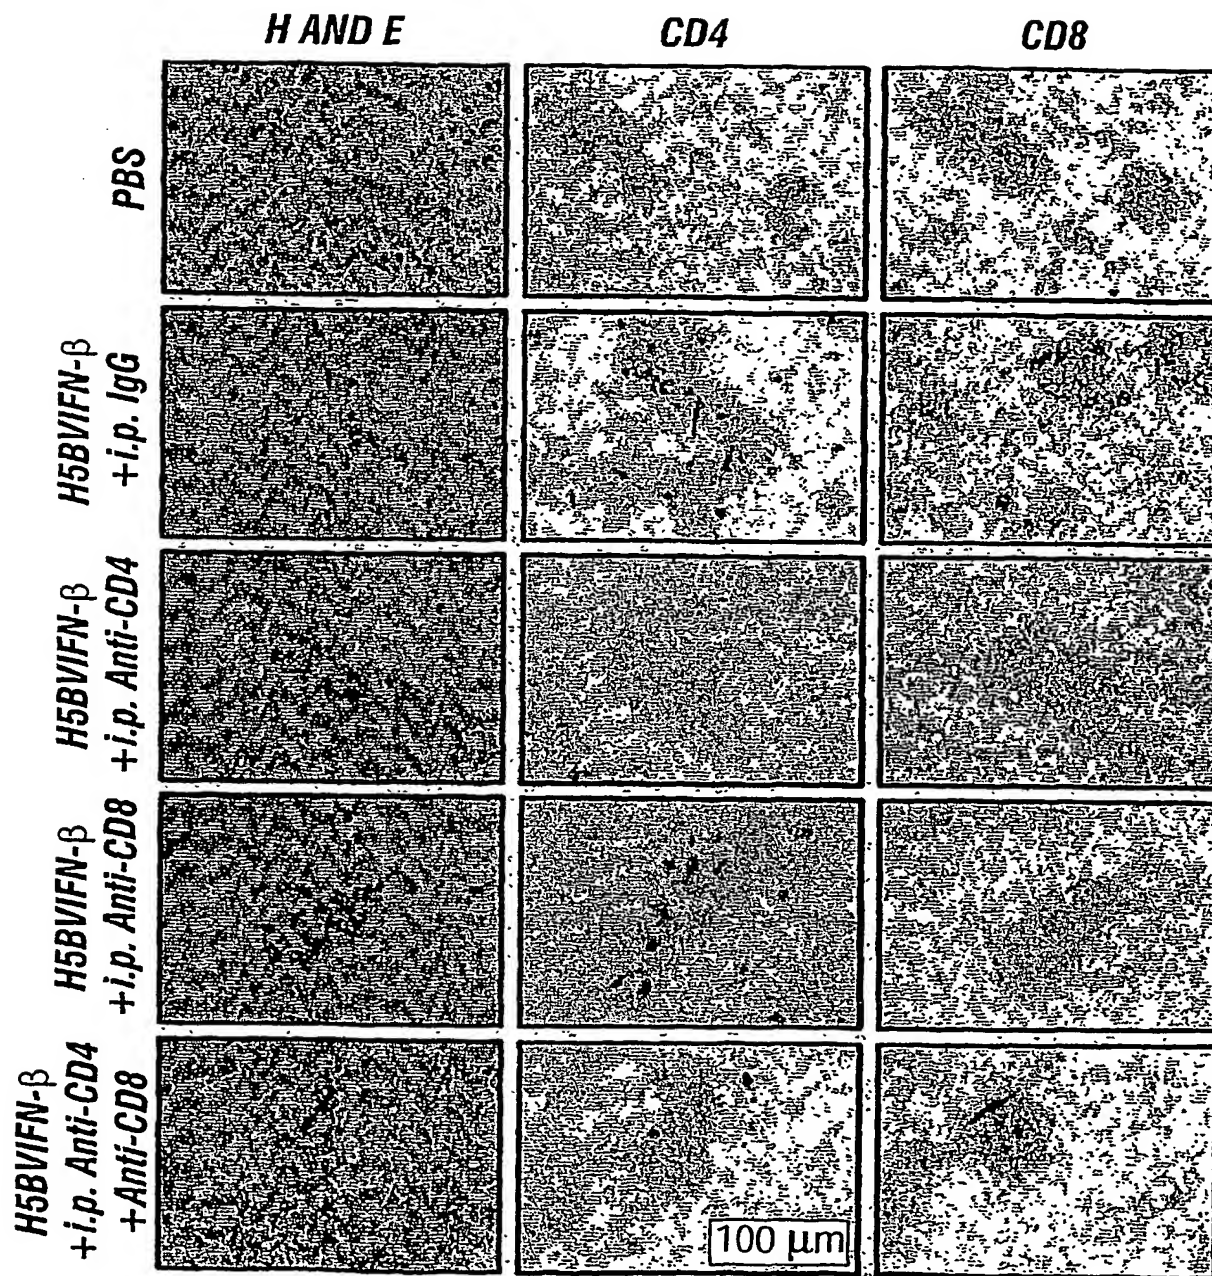

*FIG. 1*

2/14

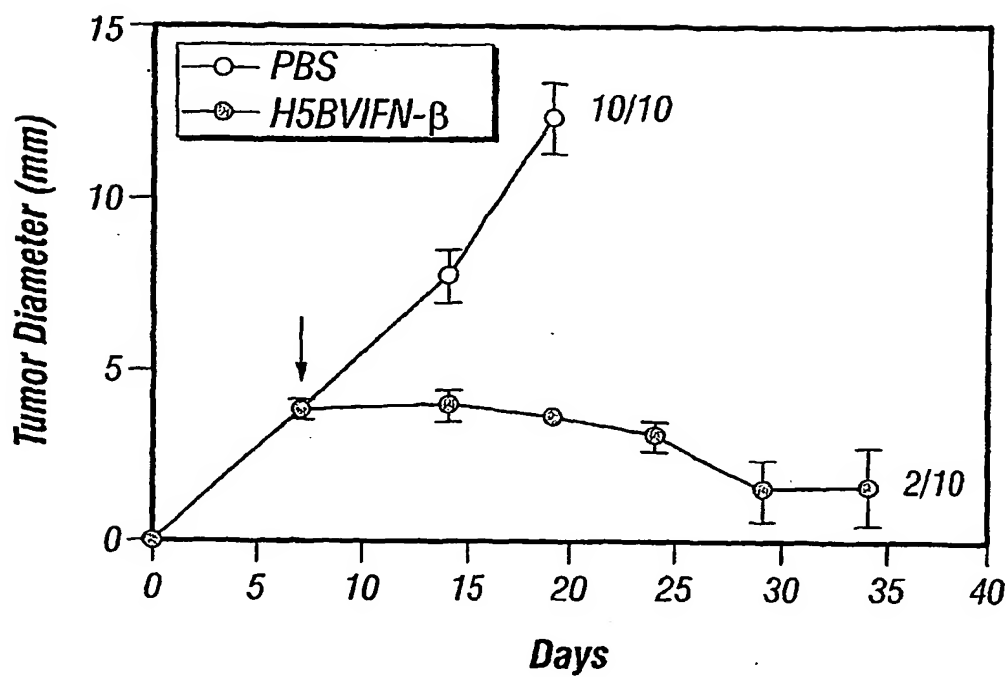


FIG. 2A

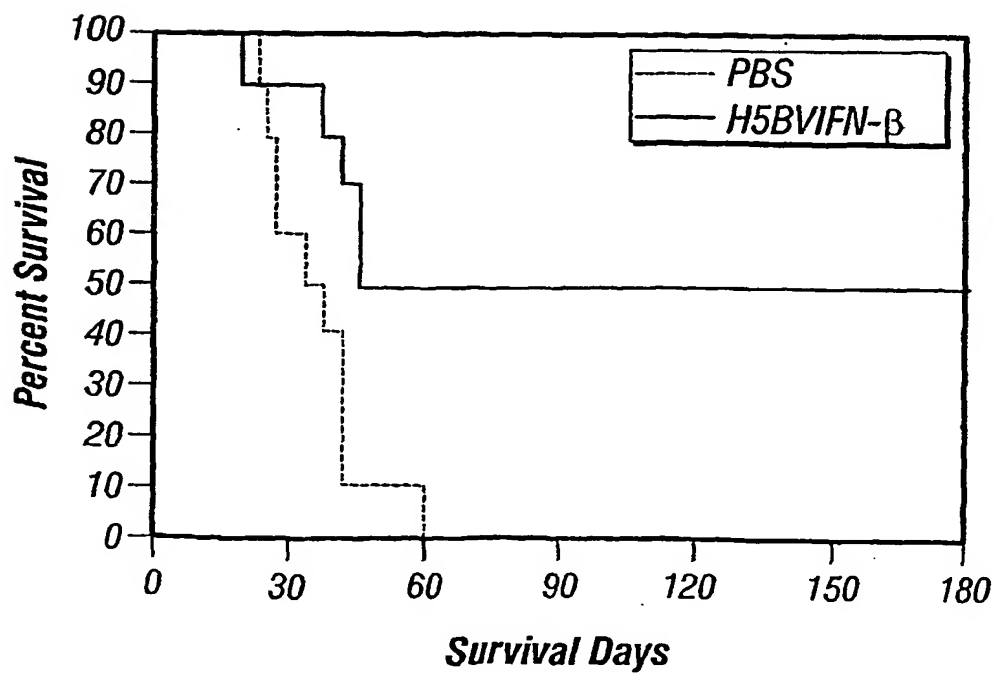


FIG. 2B

3/14

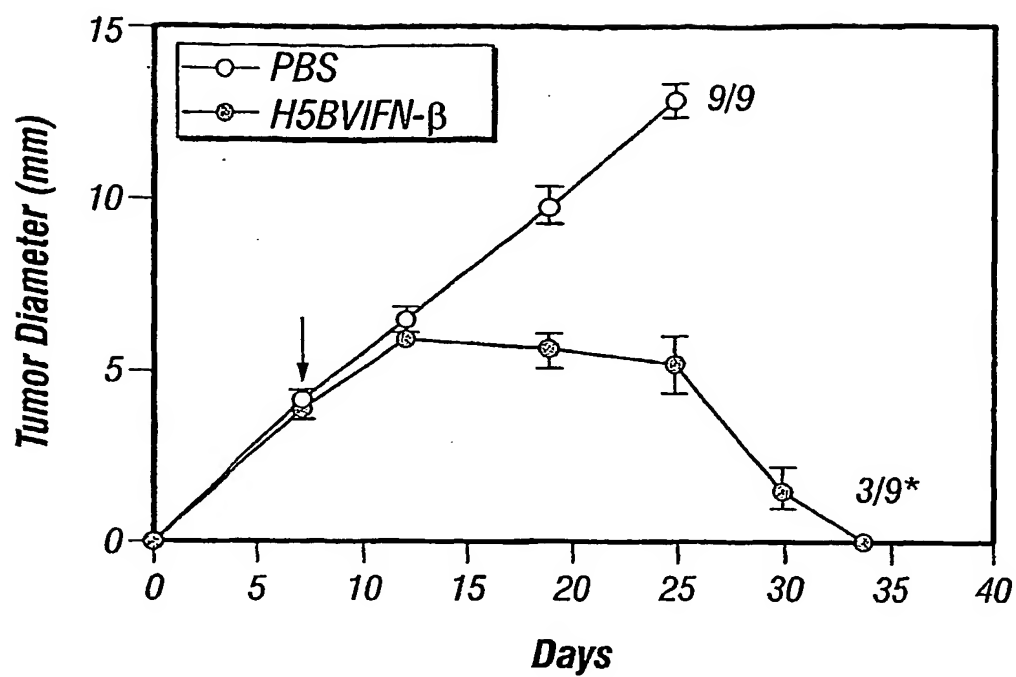


FIG. 2C


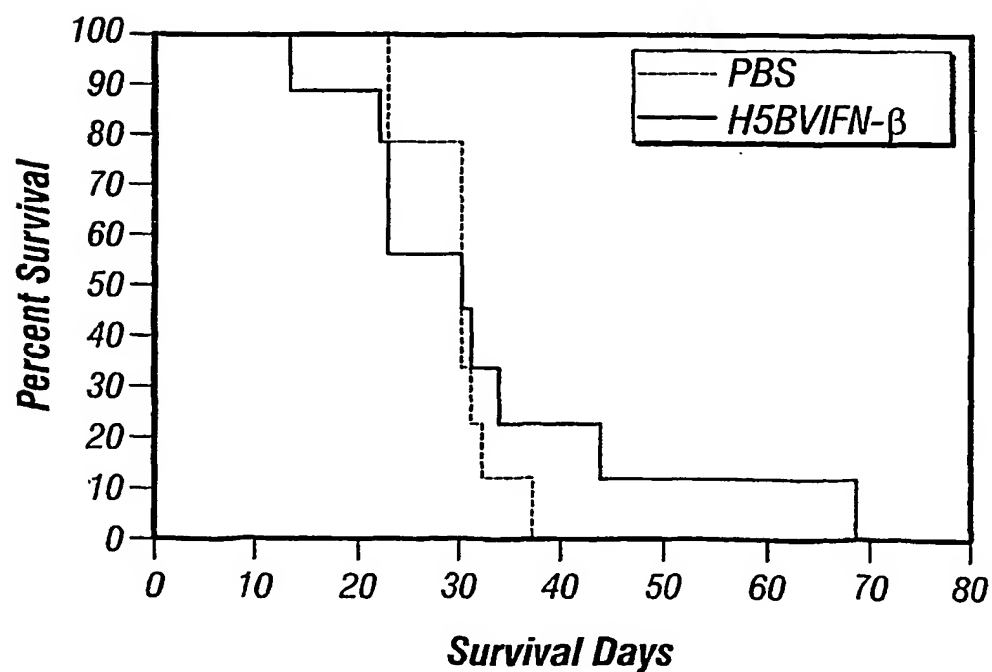


FIG. 2D

4/14

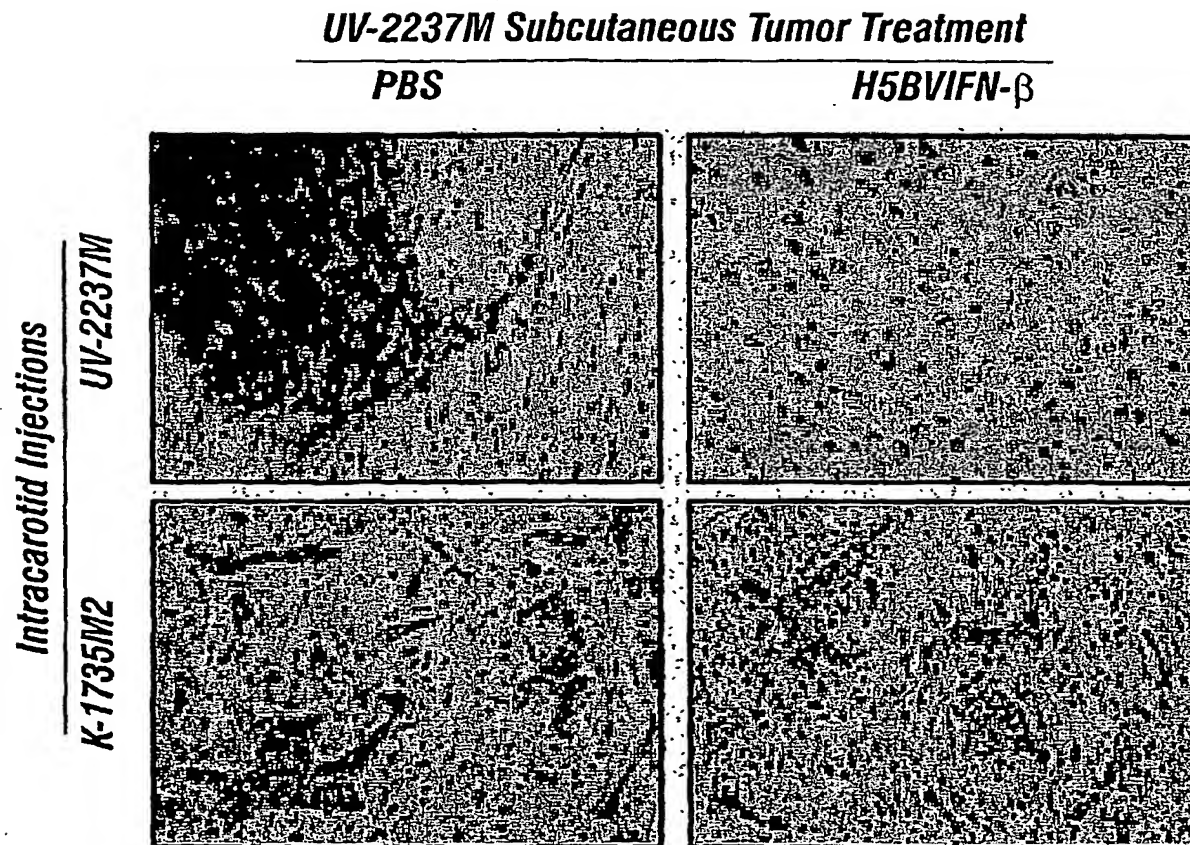

***FIG. 2E***

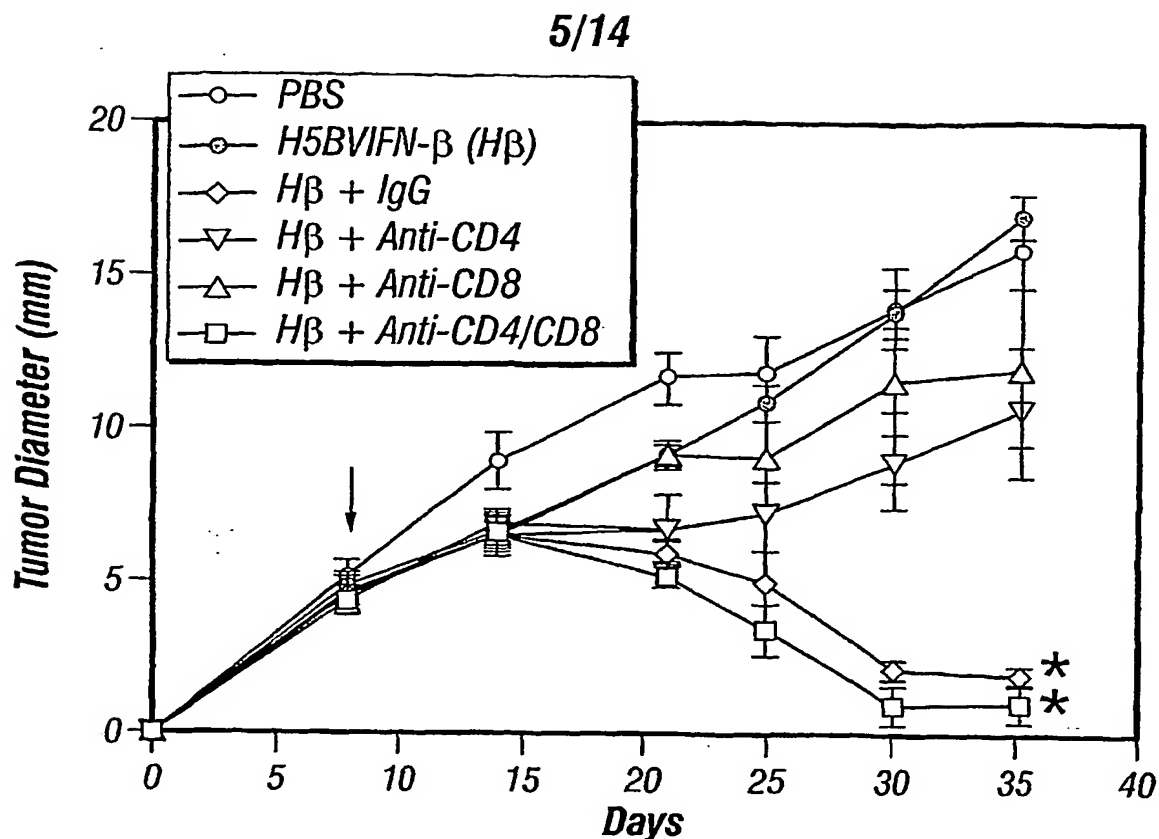


FIG. 3A

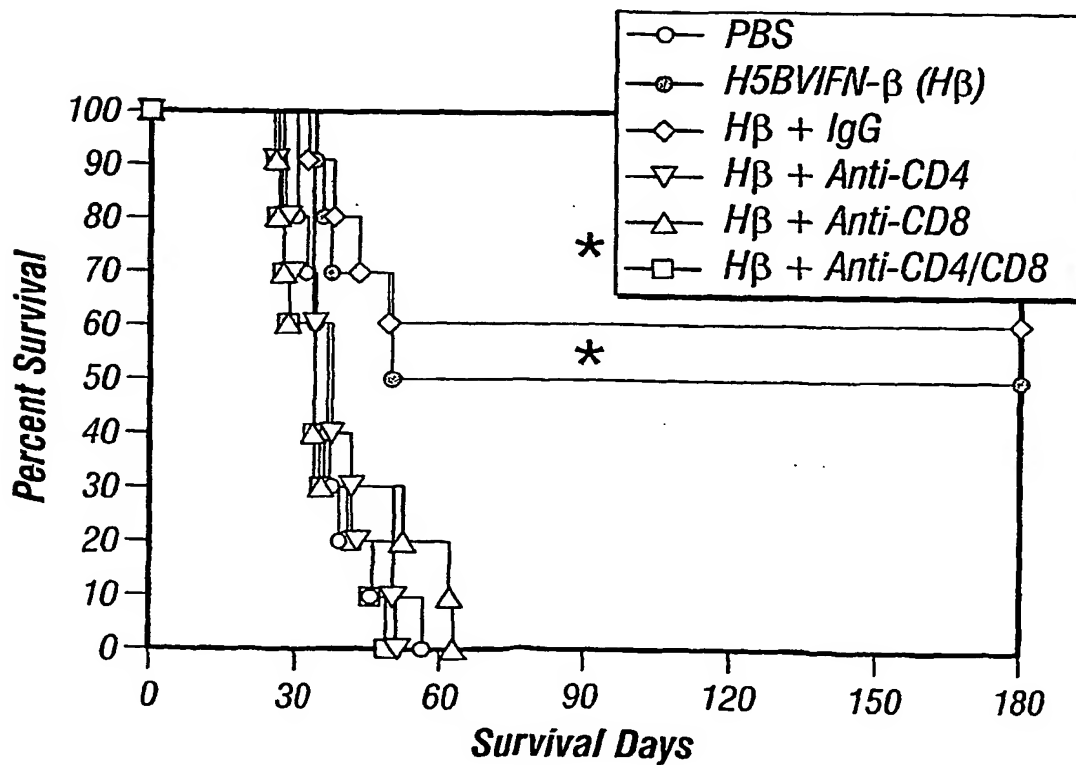
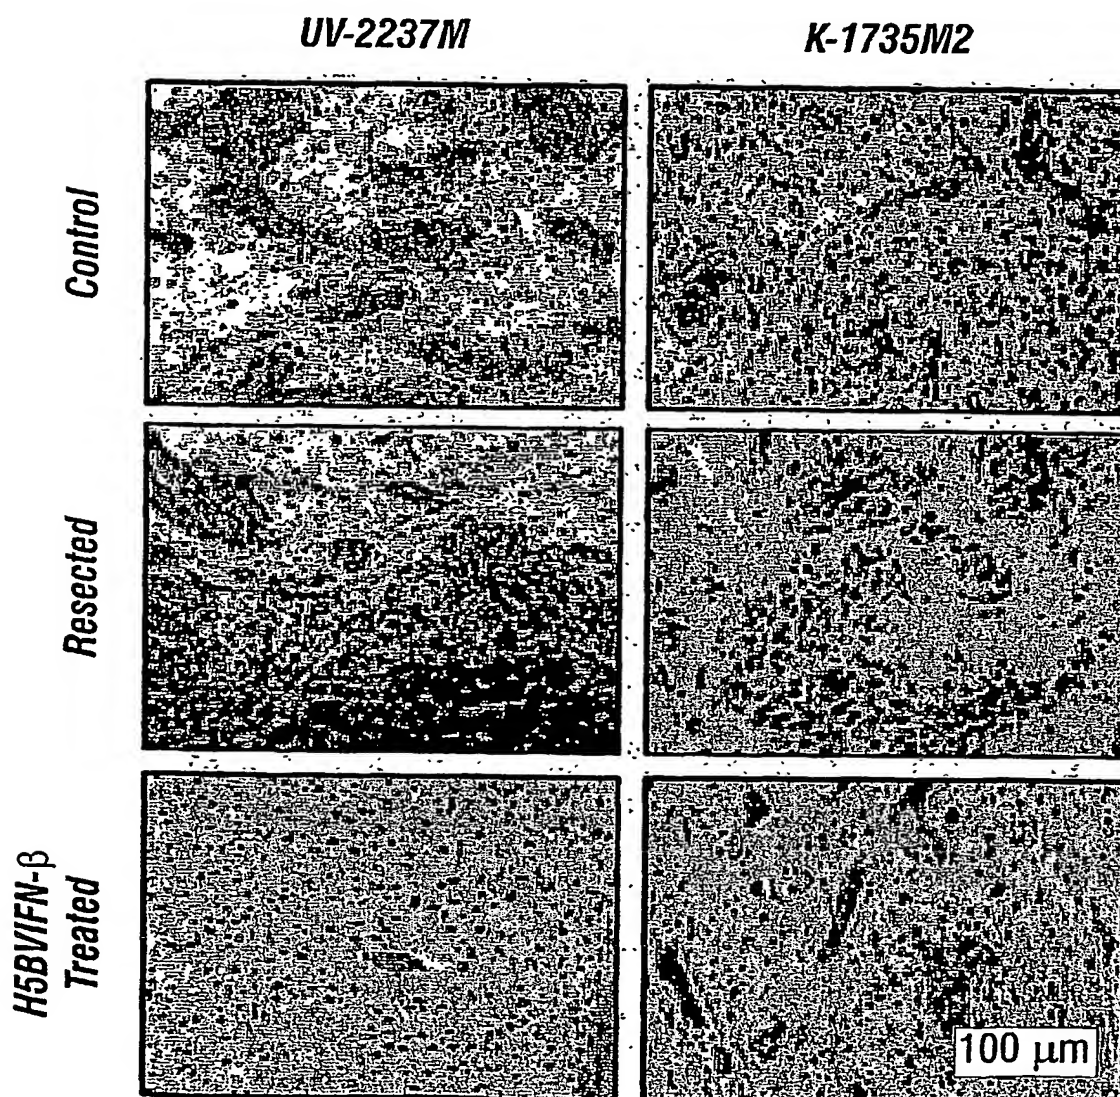


FIG. 3B

6/14

**UV-2237M Subcutaneous Tumor****Intracarotid Injections****FIG. 4A**


7/14

***K-1735M2 Subcutaneous Tumor***

***Intracarotid Injections***

***K-1735M2***

***UV-2237M***

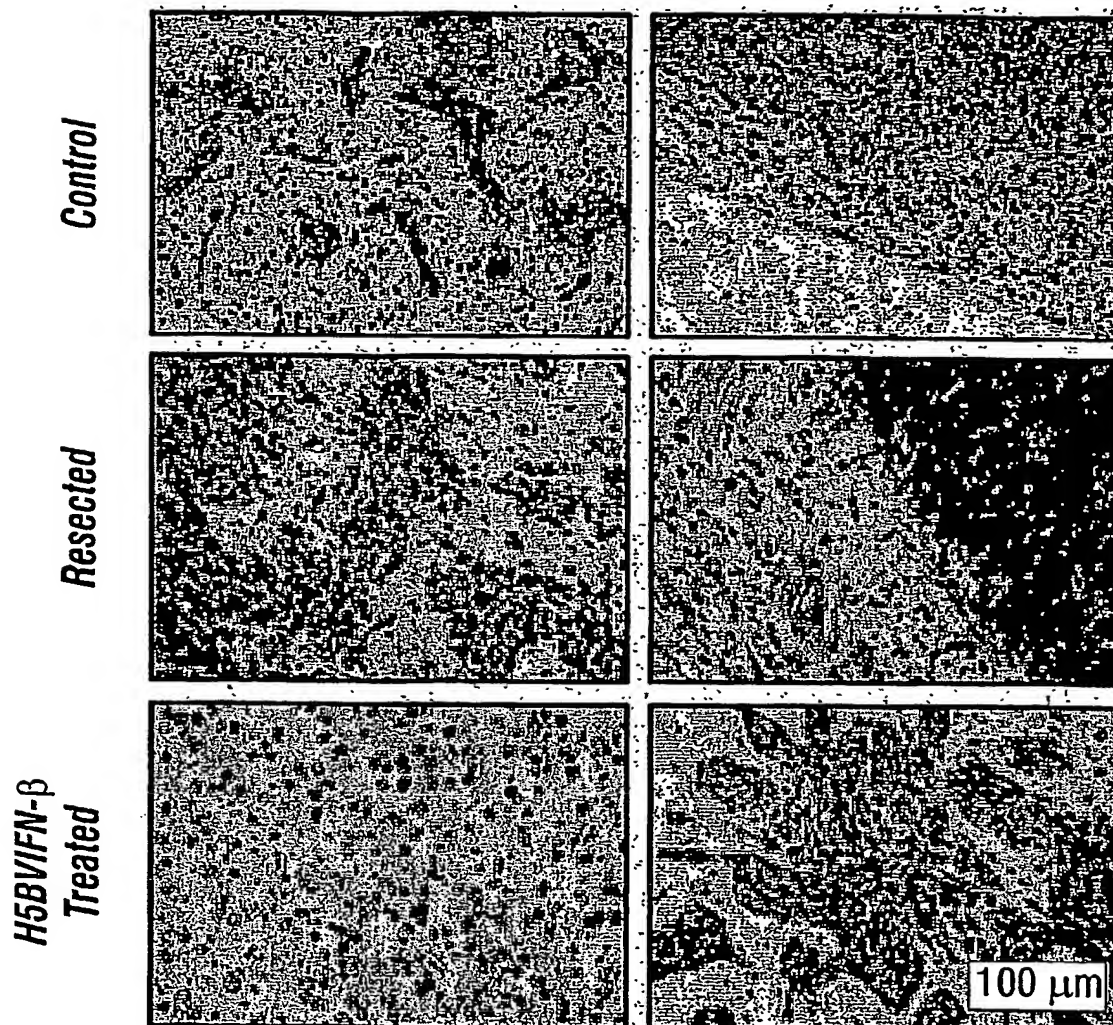

***FIG. 4B***

8/14

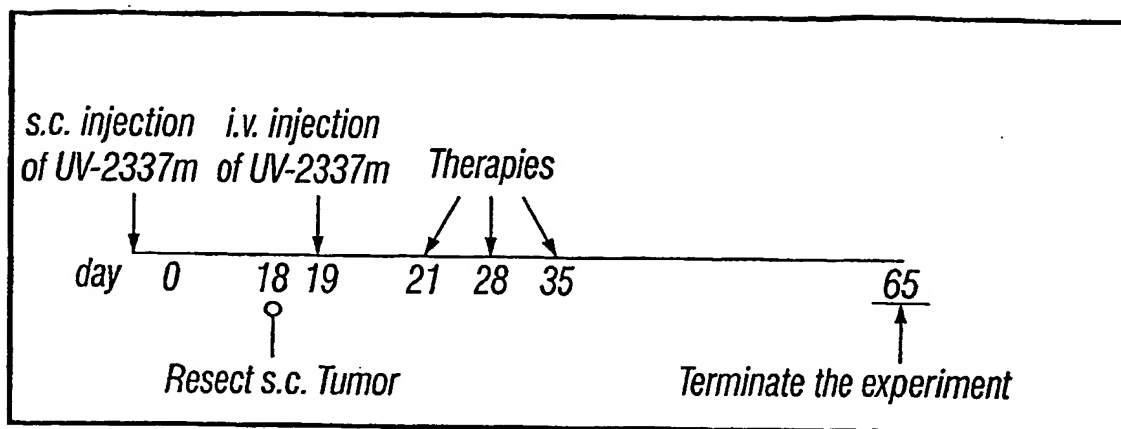


FIG. 5

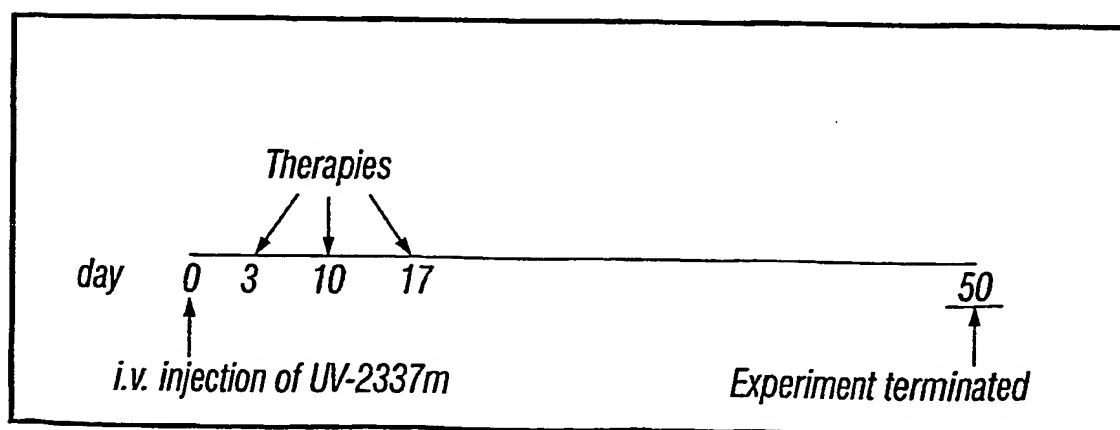


FIG. 6



9/14


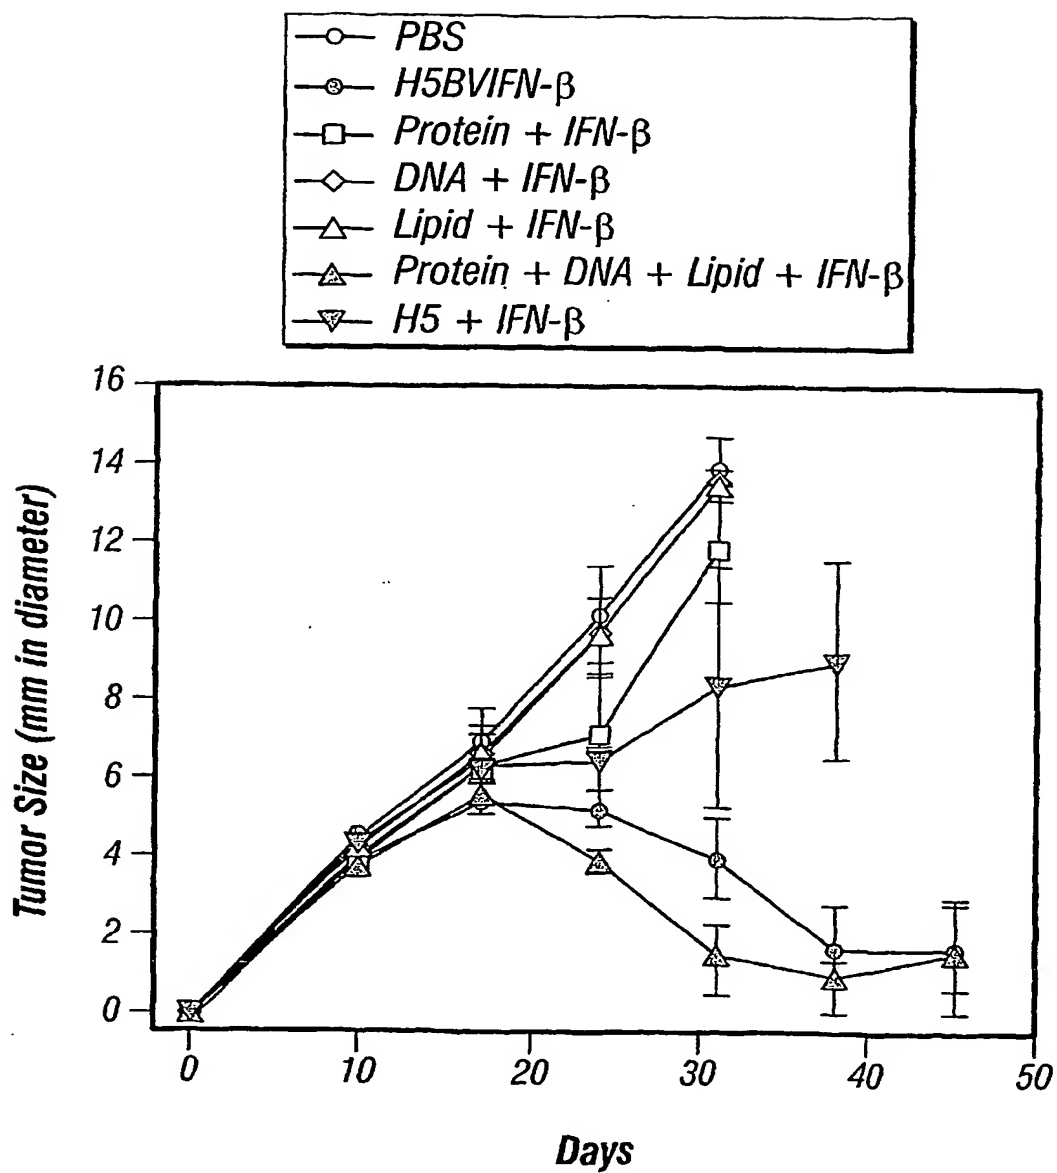


FIG. 7

**10/14**

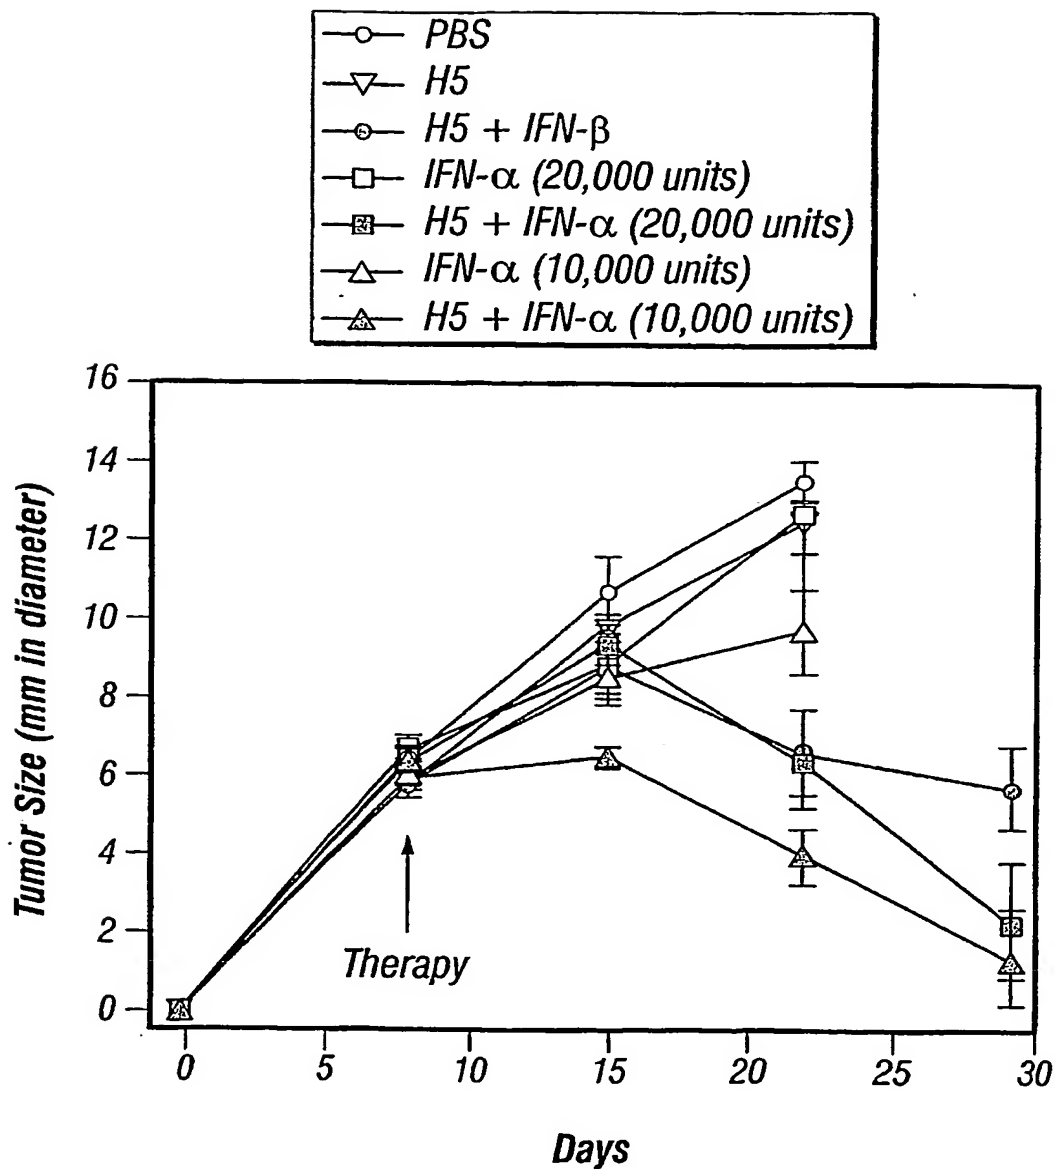

**FIG. 8**

11/14

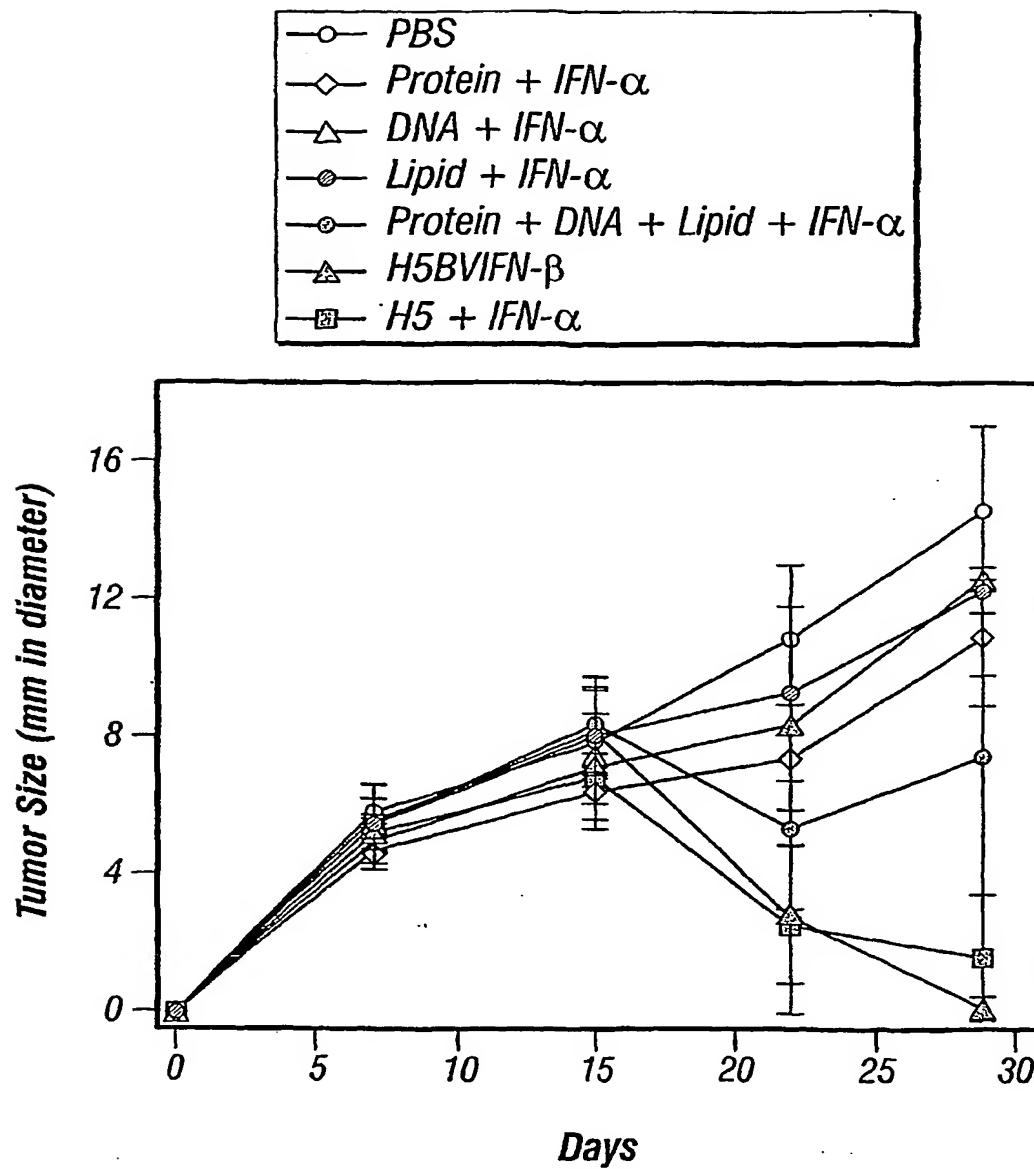


FIG. 9

12/14

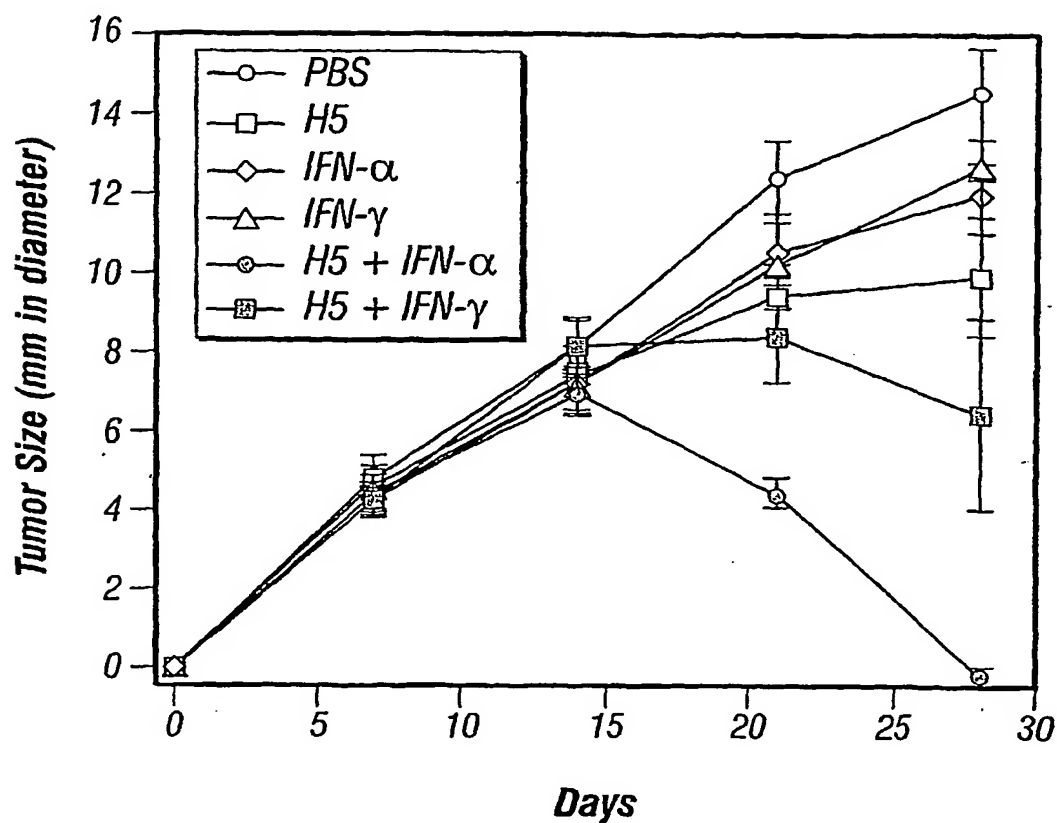


FIG. 10

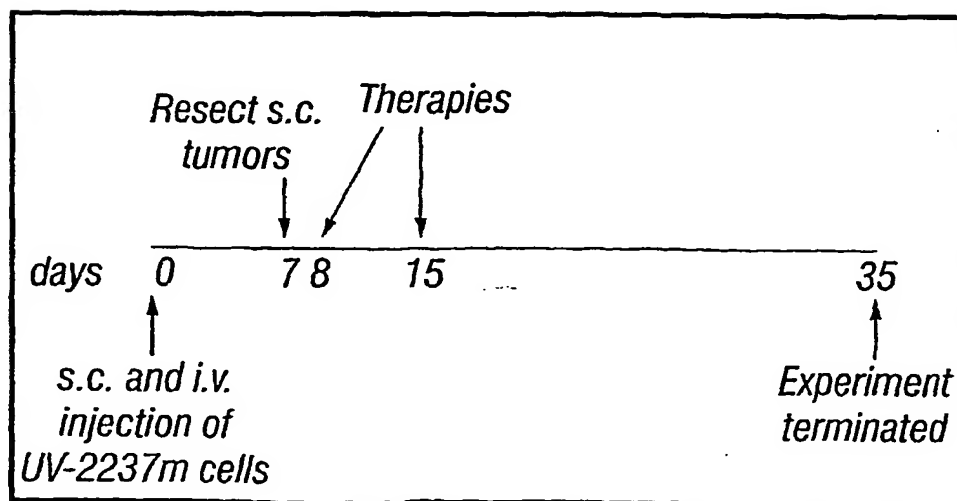


FIG. 11

13/14

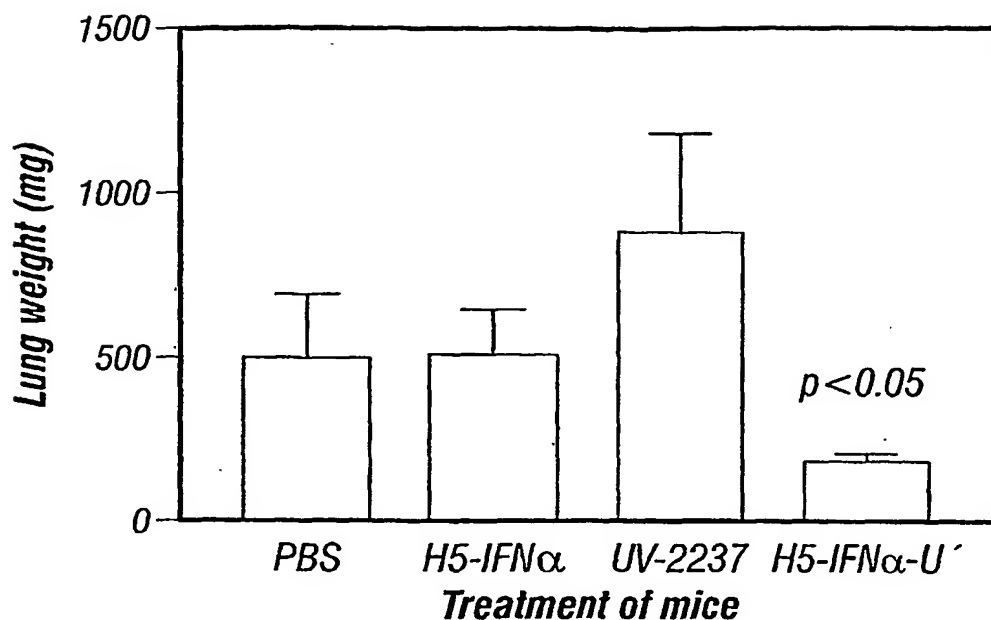


FIG. 12

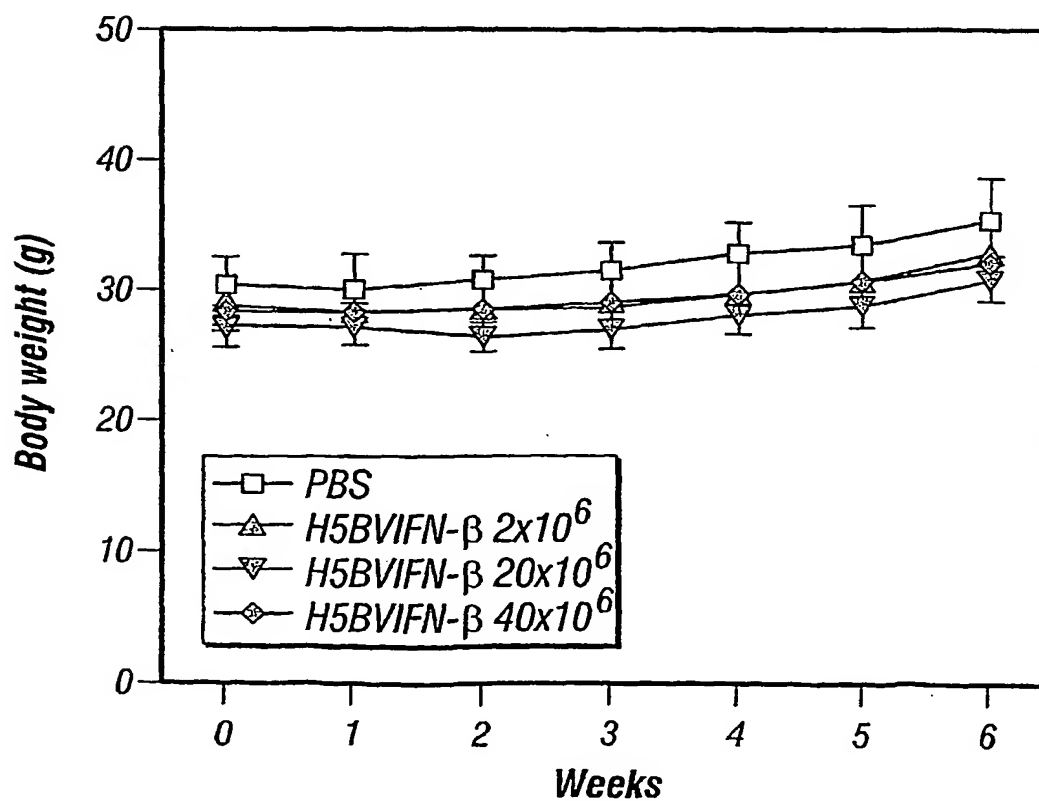


FIG. 13

14/14

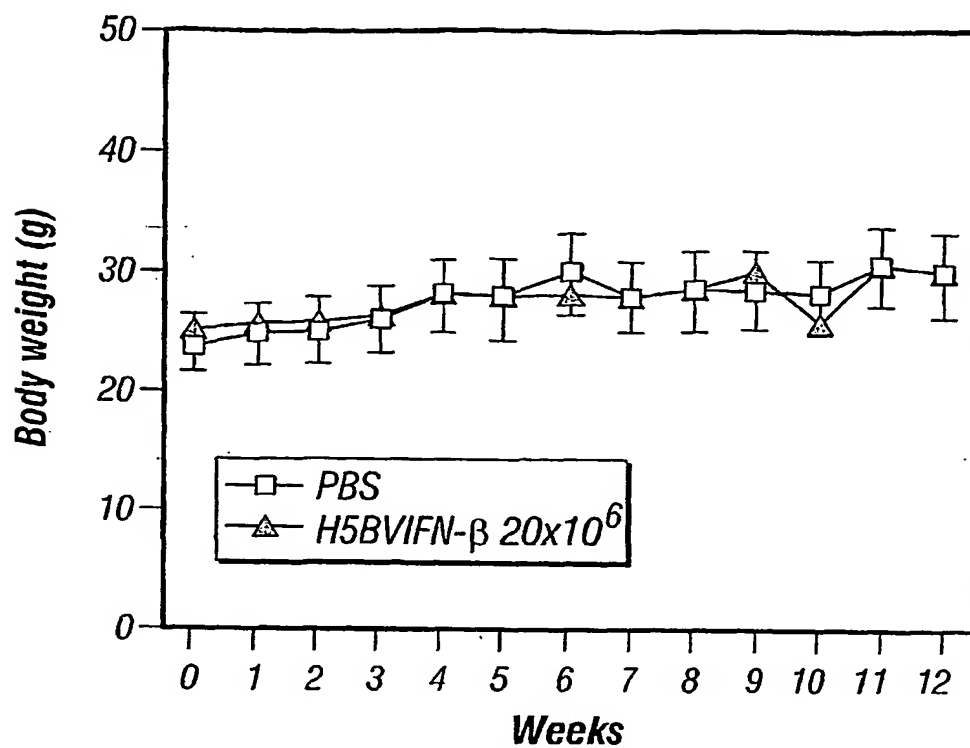


FIG. 14

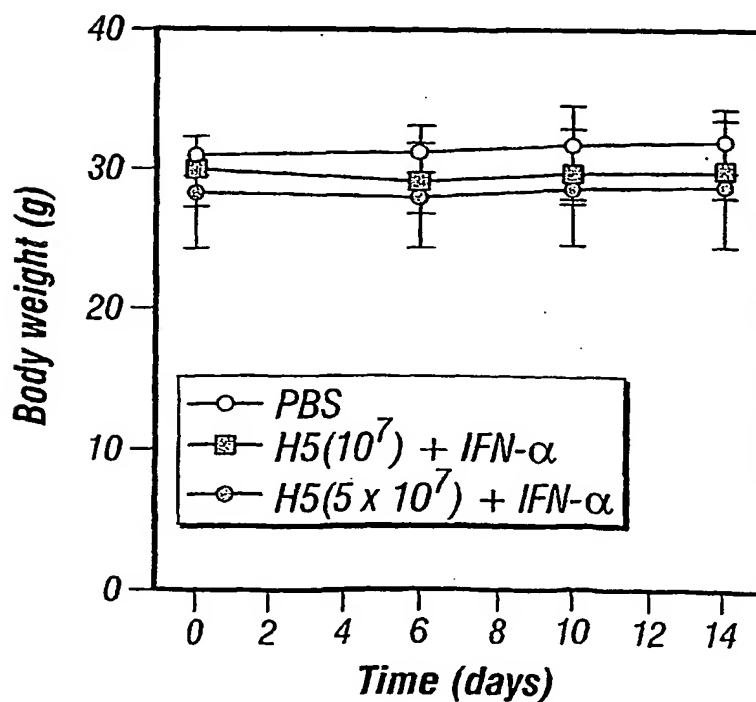


FIG. 15

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☒ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☒ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**